

## Medaval Accreditation Assessment

Volume 2016

Report 1629

05 August 2016

### **Accreditation assessment of the blood pressure measurement technology used in the Omron HEM-7252G-HP upper arm monitor, as validated according to the European Society of Hypertension International Protocol revision 2010**

#### **Approved by the Medaval Advisory Board**

Eoin O'Brien (Chair)	Yutaka Imai	Andrew Shennan
George S. Stergiou (Deputy Chair)	Martin Myers	Jan Staessen
Roland Asmar	Gbenga Ogedegbe	Martin J. Turner
Alejandro de la Sierra	Takayoshi Ohkubo	Paolo Verdecchia
Peter W. de Leeuw	Paolo Palatini	Bernard Waeber
Eamon Dolan	Gianfranco Parati	J-Guang Wang
Geoffrey A. Head		

#### **Reference**

Medaval Ltd. Accreditation assessment of the blood pressure measurement technology used in the Omron HEM-7252G-HP upper arm monitor, as validated according to the European Society of Hypertension International Protocol revision 2010. *Medical Device Assessment*. 2016 Aug 5;2016(1629). 5 p. Epub: 2019 Jan 31. Available from: <https://www.medaval.ie/MDA/2016/MDA1629.pdf>.

*Medical Device Assessment* is published by

Medaval Ltd., Unit 107, SBC, Serpentine Ave., Ballsbridge, Dublin D04 H522, IRELAND.


© 2016-2019 Medaval Ltd. All rights reserved.

**Permissions:** Requests for permissions to reproduce figures, tables, or portions of reports or articles originally published in *Medical Device Assessment* can be obtained by email request to [info@medaval.ie](mailto:info@medaval.ie).

# Accreditation assessment of the blood pressure measurement technology used in the Omron HEM-7252G-HP upper arm monitor, as validated according to the European Society of Hypertension International Protocol revision 2010

*Medaval Accreditation-Assessment Report – 5<sup>th</sup> August 2016*

### Test Device Details

		Assessment
<b>Full Name</b>	Omron HEM-7252G-HP	Requirement satisfactory
<b>Model</b>	HEM-7252G-HP	Requirement satisfactory
<b>Measurement Site</b>	Upper Arm	Requirement satisfactory
<b>Client Use</b>	Suitable for self-measurement.	Requirement satisfactory
<b>Operation Method</b>	Oscillometry, automatic during deflation	Requirement satisfactory
<b>Measurement Occurrence</b>	Single Measurements Only	Requirement satisfactory
<b>Device Photograph</b>		Photograph not in paper. Standard image shown.
<b>Manufacturer(s)</b>	Sole: Omron Healthcare, Kyoto Head Office, Shiokoji Horikawa, Shimogyo ku, Kyoto 600 8530, JAPAN.	Requirement satisfactory
<b>Cuffs</b>	Omron HEM-CS24-L: Small 17 cm to 22 cm Omron HEM-CR24-L: Medium 22 cm to 32 cm Omron HEM-RML31-L: Large 32 cm to-42 cm	Cuffs Listed: Requirement satisfactory Arm Circumferences: Requirement satisfactory

### Study Details

<b>Original Publication</b>	Takahashi H, Yoshika M, Yokoi T. Validation of two automatic devices: Omron HEM-7252G-HP and Omron HEM-7251G for self-measurement of blood pressure according to the European Society of Hypertension International Protocol revision 2010. <i>Blood Press Monit.</i> 2015 Oct; <b>20</b> (5):286-90. Epub: 2015 Apr 29. doi: 0.1097/MBP.000000000000127. PMID: 25932887.	
<b>Protocol</b>	The European Society of Hypertension International Protocol revision 2010 for the validation of blood pressure measuring devices in adults <sup>1</sup>	

		Assessment
<b>Adherence</b>	Not stated but clear from text	Requirement satisfactory
<b>Adjustments</b>	None	Requirement satisfactory
<b>Study Meas. Method</b>	Oscillometric	Requirement satisfactory
<b>Study Measurement Site</b>	Upper Arm	Requirement satisfactory
<b>Observers</b>		
<b>Supervisor + 2 Observers</b>	Yes	Requirement satisfactory
<b>Observer Training</b>	BHS online training	Requirement satisfactory
<b>Observer Familiarisation</b>	General testing	Requirement satisfactory
<b>Observer Blinding</b>	From each other	Modification: Missing “from device” accepted by review
<b>Sample</b>		
<b>Population</b>	A general population	Requirement satisfactory
<b>Circumstances</b>	None	Requirement satisfactory
<b>HBP Subjects Selection</b>	Outpatients	Requirement satisfactory
<b>NBP Subjects Selection</b>	Hospital staff & volunteers	Requirement satisfactory

<b>Test Device Details and Study Details Assessment</b>	<b>Checks</b>	22
	<b>Permitted Modifications</b>	2
	<b>Violations</b>	0

**Procedure**

**Table 1: Screening and Recruitment Details**

Screening and Recruitment				Assessment
Total Screened			<b>44</b>	Value within requirements
Total Excluded			<b>11</b>	Value within requirements
	Ranges Complete		<b>1</b>	Value within requirements
	Range Adjustment		<b>0</b>	Value within requirements
	Arrhythmias		<b>4</b>	Value within requirements
	Device Failure		<b>0</b>	Value within requirements
	Poor Quality Sounds		<b>1</b>	Value within requirements
	Cuff Size Unavailable		<b>0</b>	Value within requirements
	Observer Disagreement		<b>0</b>	Value within requirements
	Distribution		<b>0</b>	Value within requirements
	Other Reasons*		<b>5</b>	Value within requirements
Total Recruited			<b>33</b>	Value within requirements
*Explanation Summary				
The device displayed a body movement error in five individuals who were excluded for this reason.				Details satisfactory
Recruitment Ranges				
SBP	Total		<b>33</b>	Value within requirements
	Low	< 90 mmHg	<b>0</b>	Value within requirements
		90 – 129 mmHg	<b>12</b>	Value within requirements
		130 – 160 mmHg	<b>11</b>	Value within requirements
	Medium	161 – 180 mmHg	<b>6</b>	Value within requirements
		> 180 mmHg	<b>4</b>	Value within requirements
	High		<b>10</b>	Value within requirements
DBP	Total		<b>33</b>	Value within requirements
	Low	< 40 mmHg	<b>0</b>	Value within requirements
		40 – 79 mmHg	<b>11</b>	Value within requirements
		80 – 100 mmHg	<b>11</b>	Value within requirements
	Medium	101 – 130 mmHg	<b>11</b>	Value within requirements
		> 130 mmHg	<b>0</b>	Value within requirements
High		<b>11</b>	Value within requirements	
Total Extremes			<b>4</b>	Value within requirements
On Treatment Ranges				
SBP	Low	< 130 mmHg	<b>0</b>	Value within requirements
	Medium	130 – 160 mmHg	<b>2</b>	Value within requirements
	High	> 160 mmHg	<b>2</b>	Value within requirements
DBP	Low	< 80 mmHg	<b>0</b>	Value within requirements
	Medium	80 – 100 mmHg	<b>2</b>	Value within requirements
	High	> 100 mmHg	<b>2</b>	Value within requirements
<b>Table 1 Assessment</b>				
				<b>Checks</b>
				36
				<b>Permitted Modifications</b>
				0
				<b>Violations</b>
				0

### Study Results

**Table 2: Subject Details**

			<b>Assessment</b>	
Sex	Male:Female	<b>19:14</b>	Value within requirements	Value within requirements
Age (years)	Range (Low:High)	<b>28:78</b>	Value within requirements	Value within requirements
	Mean (SD)	<b>50 (12)</b>	Value within requirements	Value within requirements
Arm Circumference (cm)	Range (Low:High)	<b>20.1:37.2</b>	Value within requirements	Value within requirements
	Mean (SD)	<b>28.1 (4.6)</b>	Value within requirements	Value within requirements
Cuff for Test Device (cm)	Small (17–22)	<b>4</b>		
	Medium (22–32)	<b>23</b>		
	Large (32–42)	<b>6</b>		
	Total	<b>33</b>	Value within requirements	
Recruitment SBP (mmHg)	Range (Low:High)	<b>90:207</b>	Value within requirements	Value within requirements
	Mean (SD)	<b>144 (32.7)</b>	Value within requirements	Value within requirements
Recruitment DBP (mmHg)	Range (Low:High)	<b>48:129</b>	Value within requirements	Value within requirements
	Mean (SD)	<b>90 (20.2)</b>	Value within requirements	Value within requirements

<b>Table 2 Assessment</b>	<b>Checks</b>	19
	<b>Permitted Modifications</b>	0
	<b>Violations</b>	0

**Table 3: Observer Measurements in each Recruitment Range**

			<b>Assessment</b>	
SBP	Overall Range mmHg (Low:High)	<b>86:218</b>	Value within requirements	Value within requirements
	Low (< 130 mmHg)	<b>41</b>	Value within requirements	
	Medium (130 – 160 mmHg)	<b>28</b>	Value within requirements	
	High (> 160 mmHg)	<b>30</b>	Value within requirements	
	Maximum Difference	<b>13</b>	Value within requirements	
DBP	Overall Range mmHg (Low:High)	<b>48:134</b>	Value within requirements	Value within requirements
	Low (< 80 mmHg)	<b>26</b>	Value within requirements	
	Medium (80 – 100 mmHg)	<b>42</b>	Value within requirements	
	High (> 100 mmHg)	<b>31</b>	Value within requirements	
	Maximum Difference	<b>16</b>	Value within requirements	

<b>Table 3 Assessment</b>	<b>Checks</b>	12
	<b>Permitted Modifications</b>	0
	<b>Violations</b>	0

**Table 4: Observer Differences**

			<b>Assessment</b>	
Observer 2 – Observer 1				
SBP (mmHg)	Range (Low:High)	<b>-4:+4</b>	Value within requirements	Value within requirements
	Mean (SD)	<b>0 (1.3)</b>	Value within requirements	Value within requirements
DBP (mmHg)	Range (Low:High)	<b>-4:+4</b>	Value within requirements	Value within requirements
	Mean (SD)	<b>0 (1.3)</b>	Value within requirements	Value within requirements
Repeated Measurements		<b>0</b>	Value within requirements	

<b>Table 4 Assessment</b>	<b>Checks</b>	9
	<b>Permitted Modifications</b>	0
	<b>Violations</b>	0

**Table 5: Validation Results**

Part 1	Pass Req.		Achieved		Assessment	
	Two of	All of	SBP	DBP		
≤ 5 mmHg	73	65	<b>76</b>	<b>83</b>	Value within passing criteria	Value within passing criteria
≤ 10 mmHg	87	81	<b>92</b>	<b>97</b>	Value within passing criteria	Value within passing criteria
≤ 15 mmHg	96	93	<b>97</b>	<b>99</b>	Value within passing criteria	Value within passing criteria
Grade 1			<b>Pass</b>	<b>Pass</b>	Value within passing criteria	Value within passing criteria
Mean mmHg			<b>-1.5</b>	<b>-1.2</b>	Value within requirements	Value within requirements
SD mmHg			<b>5.1</b>	<b>3.9</b>	Value within requirements	Value within requirements



Part 2	Pass Req.	Achieved		Assessment	
		SBP	DBP		
2/3 ≤ 5 mmHg	≥ 24	<b>28</b>	<b>29</b>	Value within passing criteria	Value within passing criteria
0/3 ≤ 5 mmHg	≤ 3	<b>1</b>	<b>2</b>	Value within passing criteria	Value within passing criteria
Grade 2		<b>Pass</b>	<b>Pass</b>	Value within passing criteria	Value within passing criteria
Grade 3		<b>Pass</b>	<b>Pass</b>	Value within passing criteria	Value within passing criteria

Part 3	Result	Pass	Value within passing criteria
Table 5 Assessment			

<b>Table 5 Assessment</b>	<b>Checks</b>	21
	<b>Permitted Modifications</b>	0
	<b>Violations</b>	0

**Plots**

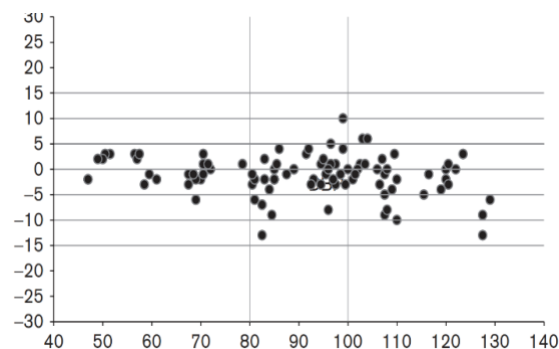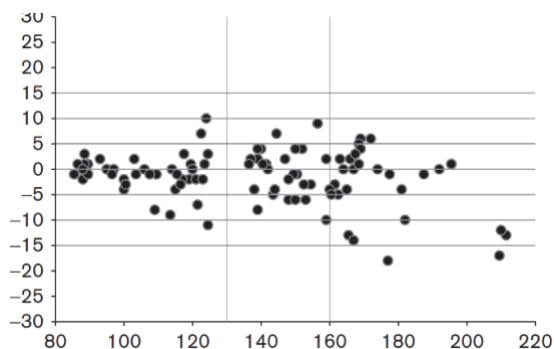

SBP Plot Provided **Yes**  
 DBP Plot Provided **Yes**

Requirement satisfactory  
 Requirement satisfactory

<b>Plots Assessment</b>	<b>Checks</b>	2
	<b>Permitted Modifications</b>	0
	<b>Violations</b>	0

**Recommendations**

**Overall Summary**

Number of checks 121  
 Number of permitted modifications 2  
 Number of violations 0

**Assessment Summary**

The validation has been checked and is verified as having been conducted in accordance with the protocol requirements. Therefore, the results are considered to be valid, the null hypothesis, that the device is inaccurate in measuring blood pressure, is rejected and the conclusion, that the device is accurate for self-measurement in adults, is correct.

**Certification Decision**

The Omron HEM-7252G-HP, with the HEM-CR24-L: medium 22 cm to 32 cm or HEM-RML31-L: large 32 cm to 42 cm is certified by Medaval Ltd., for blood pressure measurement in adults, as it fulfilled the conditions required for a pass in a validation study carried out in accordance with the requirements of the International Protocol of the European Society of Hypertension 2010 Revision.

Date of Advisory Board Approval: 29<sup>th</sup> July 2016.

**Reference**

- O'Brien E, Atkins N, Stergiou G, Karpettas N, Parati G, Asmar R, Imai Y, Wang J, Mengden T, Shennan A; Working Group on Blood Pressure Monitoring of the European Society of Hypertension. European Society of Hypertension International Working Protocol revision 2010 for the validation of blood pressure measuring devices in adults. *Blood Press Monit.* 2010;15:23-38. doi: 10.1097/MBP.0b013e3283360e98. PMID: 20110786. Erratum in *Blood Press Monit.* 2010;15(3):171-2.