

OMRON


INSTRUCTION MANUAL



Automatic Wrist Blood Pressure Monitor

自动手腕式电子血压计

Model
型号 **HEM-6052**

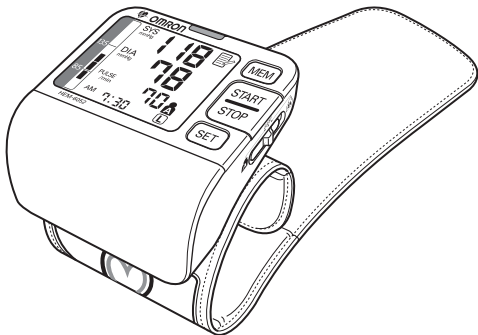

A Good Sense of Health

Contents

Before using the unit

Introduction	3
Important Safety Information	4
1. Overview	6
2. Preparation	8
2.1 Installing/Replacing the Batteries.....	8
2.2 Setting the Date and Time	10
2.3 Setting the Advanced Positioning Sensor (APS)	12

Operating instructions

3. Using the Monitor.....	15
3.1 Applying the Wrist Cuff.....	15
3.2 Taking a Reading.....	17
3.3 Using the Memory Function	22

Care and maintenance

4. Handling Errors and Problems	24
5. Storage and Maintenance.....	26
6. Technical Data.....	27
7. Some Useful Information about Blood Pressure.....	29

Introduction

Thank you for purchasing the HEM-6052 Wrist Blood Pressure Monitor.

This remarkable, compact and easy to use instrument is ideal for people who frequently monitor their own blood pressure. The small, pre-formed wrist cuff is very convenient and easy to apply.

With the push of a button the HEM-6052 measures your blood pressure and pulse and displays the reading on a clear digital panel. Perfect for quick, easy readings at home, at work, and while travelling. It also stores up to 100 sets of measurements in memory and displays an average reading based on the three most recent measurements.

The HEM-6052 uses the oscillometric method of blood pressure measurement. This means the monitor detects the pulse wave vibrations in the artery of your wrist and converts the oscillations into a digital reading.

Clinical research has proven a direct relationship between blood pressure in the wrist and blood pressure in the arm. Changes in wrist blood pressure reflect changes in arm blood pressure because the arteries in the wrist and the arm are connected.

Frequently measuring the blood pressure in your wrist will provide you and your doctor with an accurate indication of changes in your true blood pressure.



Please read this instruction manual thoroughly before using the unit. For specific information about your own blood pressure, CONSULT YOUR DOCTOR.

Important Safety Information

Consult your doctor during pregnancy, arrhythmia and arteriosclerosis. People with poor peripheral circulation may find that results for measurements taken at the wrist vary from those taken on the upper arm. Please read this section carefully before using the unit.

Warning:

Indicates a potentially hazardous situation which, if not avoided, could result in death or serious injury.

(General Usage)

- Always consult your doctor. Self-diagnosis of measurement results and self-treatment are dangerous.
- People with severe blood flow problems, or blood disorders, should consult a doctor before using the unit. Cuff inflation can cause internal bleeding.

(Battery Usage)

- If battery fluid should get in your eyes, immediately rinse with plenty of clean water. Consult a doctor immediately.

Caution:

Indicates a potentially hazardous situation which, if not avoided, may result in minor or moderate injury to the user or patient or damage to the equipment or other property.

(General Usage)

- Do not leave the unit unattended with infants or persons who cannot express their consent.
- Do not use the unit for any purpose other than measuring blood pressure.
- Do not disassemble the unit or wrist cuff.
- Do not inflate the wrist cuff over 299 mmHg.

- Do not use a mobile phone, or other devices that emit electromagnetic fields, near the unit. This may result in incorrect operation of the unit.
- Do not operate unit in a moving vehicle (car, airplane).

(Battery Usage)

- If battery fluid should get on your skin or clothing, immediately rinse with plenty of clean water.
- Use only two “AAA” alkaline (LR03) batteries with this unit. Do not use other types of batteries.
- Do not insert the batteries with their polarities incorrectly aligned.
- Replace old batteries with new ones immediately. Replace both batteries at the same time.
- Remove the batteries if the unit will not be used for three months or more.
- When the batteries are replaced, you may need to reset the date and time. If the year is flashing on the display screen, refer to “2.2 Setting the Date and Time”.
- Do not use new and used batteries together.


General Safety Precautions

- Do not inflate the wrist cuff when it is not wrapped around your wrist.
- Do not apply strong shocks and vibrations to or drop the unit.
- Do not take measurements after bathing, drinking alcohol, smoking, exercising or eating.
- Do not wash the wrist cuff or immerse it in water.

Save these instructions for future reference.

1. Overview


Main Unit

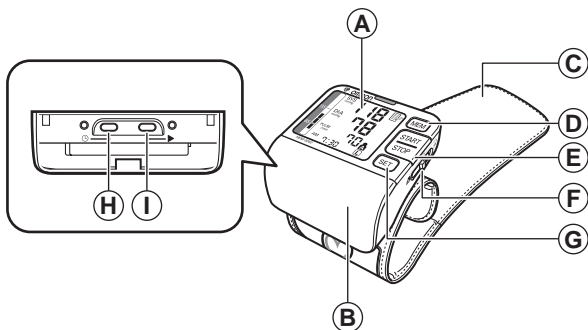

- A. Display
- B. Battery compartment
- C. Wrist cuff
- D. Memory (MEM) button
- E. START/STOP button

- F. User ID selection switch
- G. SET button
- H. Date/Time setting (⌚) button
- I. Date/Time setting (▶) button


Package contents



- J. Two “AAA” alkaline (LR03) batteries
- K. Storage case

- Instruction manual
- Quick reference guide

Display

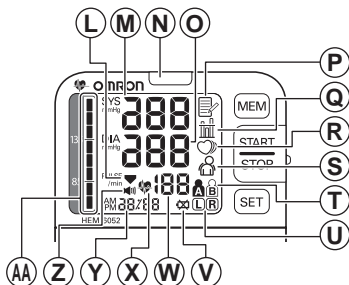


- | | |
|--|---|
| L. Deflation symbol | T. User ID symbol (A or B)
(If "GUEST" is selected, A or B will not be displayed.) |
| M. Systolic blood pressure | U. Wrist symbol |
| N. Positioning indicator | V. Battery low symbol |
| O. Diastolic blood pressure | W. Pulse display |
| P. Memory symbol
(Displayed when viewing values stored in memory) | X. Heartbeat symbol
(Flashes during measurement) |
| Q. Average value symbol
(Refer to section 3.3.) | Y. Date/Time display |
| R. Irregular heartbeat symbol | Z. Buzzer symbol |
| S. Movement error symbol
(Displayed if you move your body during the measurement) | AA. Blood pressure level indicator |


2. Preparation

2.1 Installing/Replacing the Batteries

1. Remove the battery cover by pulling it off in the direction of the arrow.




2. Insert two 1.5V “AAA” alkaline (LR03) batteries in the battery compartment. Make sure their polarity (+/-) is aligned with the polarity (+/-) as indicated in the battery compartment.




3. Set the date and time. Refer to section 2.2.


4. Put the battery cover back in place.



Note: Make sure that the battery cover is securely in position.



Battery Life & Replacement



If the battery low symbol () appears on the display, replace both batteries at the same time.

- When the battery low symbol () starts to blink, you will still be able to use the unit for a short while. You should replace the batteries with new ones ahead of time.
 - When the symbol () remains lit, the batteries were exhausted. You should replace the batteries with new ones at once.
- Turn the unit off before replacing the batteries.
 - Remove the batteries if the unit will not be used for three months or more.
 - If the batteries are removed, the Date/Time setting will need to be reset. See “2.2 Setting the Date and Time” for details.
 - Dispose of batteries according to applicable local regulations.
 - Two new identical 1.5V “AAA” alkaline (LR03) batteries will last for approximately 300 measurements, when used to take two measurements a day.
 - Since the supplied batteries are for monitoring use only, they may have a shorter life and not last for 300 measurements.

2.2 Setting the Date and Time


Your blood pressure monitor automatically stores up to 100 measurement values in its memory and calculates an average value based on the last three measurements. To make use of the memory and average value function:

- Set the monitor to the correct date and time before taking a measurement for the first time.
- If the batteries have been removed for a long period of time, the date and time setting will need to be reset.

1. Press the Date/Time setting (⌚) button. The year digits (2009) will flash on the display.


Notes:

- The range for the year setting is 2009 to 2030. If the year reaches 2030, it will return to 2009.
- If you need to reset the date and time, press the ⌚ button until the setting you want to adjust appears on the display, then press the Date/Time setting (▶) button to change the setting.




2. Press the ▶ button to advance the digits one at a time.



Note: If you hold down the ▶ button, the digits will advance rapidly.





3. Press the ⌚ button to confirm the setting when the desired number appears on the display. The year setting is set and the month digits will flash.



4. Repeat steps 2 and 3 to set the month and day.



5. Repeat steps 2 and 3 to set the hour and minute for the time.



6. Press START/STOP button to turn the monitor off.


2.3 Setting the Advanced Positioning Sensor (APS)

You can modify the options for the various settings of your monitor. This is done by pressing the SET button to changing a setting, then pressing the MEM button to select the options for that setting. After selecting a setting, press the START/STOP button to confirm the setting and turn the power off.


Setting the Positioning Indicator

1. Select your User ID. Press the SET button.

Note: The default setting is “on1”.

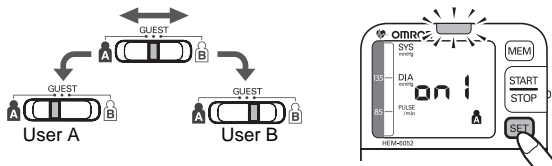

2. Press the MEM button to select the Positioning indicator “on1”, “on2”, or “off”.

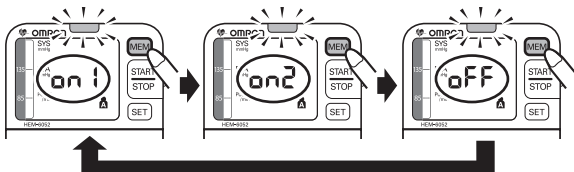


- on1: After the Positioning indicator lights in blue for more than 2 seconds, or in orange for more than 5 seconds, measurement starts automatically, even though the monitor is not in the proper position.
- on2: The Positioning indicator lights in blue for more than 2 seconds, measurement starts automatically. Measurement will not start if it lights in orange.
- off: Measurement starts without the Positioning indicator.

Setting the Wrist for Measurement


1. While in the setting mode, press the SET button until the wrist symbol (L or R) appears on the display.

Notes:

- The default setting is “L”.
- After you choose “oFF” for the Positioning indicator, the monitor skips this process.




2. Press the MEM button to select the left wrist (L) or the right wrist (R).

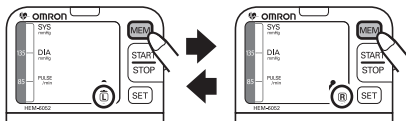


Setting the Buzzer

1. While in the setting mode, press the SET button until the buzzer symbol (🔊) appears on the display.

Note: The default setting is “on1” or “on”, depending on the Positioning indicator you set.



2. Press the MEM button to select the buzzer setting.

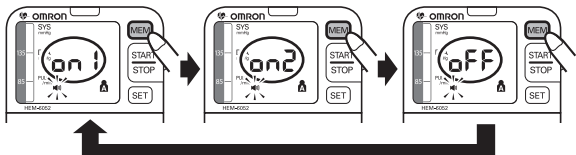

If the Positioning indicator is “on1” or “on2”:

on1: The buzzer sounds only when the monitor is in proper position.

on2: The buzzer sounds a series of two short blips if your wrist is too far away from the measuring position, and beeps when your wrist is in the proper position.

off: The buzzer will not sound.

If the Positioning indicator is “off”:

on: The buzzer sounds when pressing any buttons.

off: The buzzer will not sound.

Resetting to the Default Setting

The positioning indicator is set “on1”, the wrist for measurement is set “L”, and the buzzer is set “on1” as default.

To reset to the default setting, press and hold the SET button while in the setting mode, then press the START/STOP button simultaneously for more than 2 seconds.

3. Using the Monitor

3.1 Applying the Wrist Cuff

You can take a measurement on either your left or right wrist.


Notes:

- You can take a measurement on either your left or right wrist. The blood pressure can differ between your right and left wrist and therefore also the measured blood pressure values can be different. Omron recommends to always use the same wrist for a measurement. If the values between the two wrists differ substantially, please check with your doctor which wrist to use for your measurement.
- To ensure correct measurement, apply the wrist cuff so that it fits comfortably around your wrist.
- Roll up your sleeve so that the unit covers bare skin.
- Do not apply over clothing.



Taking a reading on the left wrist

1. Roll up your sleeve so that the monitor covers bare skin. Do not apply over clothing.

Make sure that your sleeve is not too tight and does not constrict the flow of blood in your arm.



2. Place the wrist cuff over your left wrist with your left thumb facing upward.



Note: Make sure that the wrist cuff does not cover the protruding part of the wrist bone (ulna) on the outside of the wrist.

3. Hold the bottom part of the wrist cuff and wrap it around the wrist while pulling so that it fits comfortably.




Unless the wrist cuff is wrapped securely around the wrist, it may not be possible to take correct measurements.

Taking measurements on the right wrist

Measurements can also be made on the right wrist.

Fit the monitor on the right wrist as shown.


Refer to 2.3 about how to modify the settings.



3.2 Taking a Reading


Note: This section is the example for the measurement with the default setting (the positioning indicator is “on1”, the wrist for measurement is “L”, and the buzzer is “on1”).

1. Select your User ID.
Always use the same user ID when taking a measurement. The unit stores the measurement values in the selected user ID memory.
Slide the User ID selection switch to select user A or B.



Note: If you select the GUEST, the measurement values are not stored in the memory.


2. Press the START/STOP button.



3. Keep the heart mark on the wrist cuff at the center of the chest.





Sit upright with your back straight.



Do not hold the wrist with the other hand.

Relax.

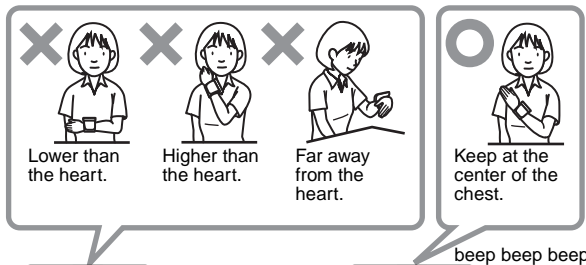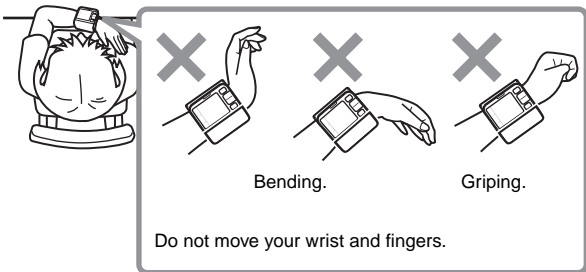

The orange light



The blue light

While your position is improper, the Positioning indicator lights in orange, when you are in proper position the buzzer beeps “beep beep beep” and the Positioning indicator turns to blue. Then the wrist cuff automatically starts to inflate and measurement starts.


The Positioning indicator will light in the same color, after measurement completed or when viewing results stored in the memory.

Notes:


- Sit still and do not talk or move until the measurement is completed.
- Keep the monitor at heart level until the measurement is completed.
- To cancel the measurement, press the START/STOP button at any time during measurement.

4. After the monitor has detected your blood pressure and pulse rate, the buzzer sounds “beep pip pip pip”. The cuff automatically deflates and your blood pressure and pulse rate are displayed.

Note: The time and date of the measurement are displayed alternately.




5. Press the START/STOP button to turn the monitor off.
If you forget to turn the monitor off, it will shut itself off automatically after two minutes.






Important:


- Recent research suggests that the following values can be used as a guide to high blood pressure for measurements taken at home.


Systolic Blood Pressure	Above 135 mmHg
Diastolic Blood Pressure	Above 85 mmHg




This criteria is for home blood pressure measurement. For professional office blood pressure measurement criteria, please refer to Chapter 7 “Some Useful Information about Blood Pressure”.

- Your blood pressure monitor includes an irregular heartbeat feature. Irregular heartbeats can influence the results of the measurement. The irregular heartbeat algorithm automatically determines if the measurement is usable or needs to be repeated. If the measurement results are affected by irregular heartbeats but the result is valid, the result is shown together with the irregular heartbeat symbol (). If the irregular heartbeats cause the measurement to be invalid, no result is shown. If the irregular heartbeat symbol () is shown after you have taken a measurement, repeat the measurement. If the irregular heartbeat symbol () is shown frequently, please make your doctor aware of it.





- If you move during measurement, the movement error symbol () will appear on the display. Keep still and repeat the measurement.



What is Irregular Heartbeat?

An irregular heartbeat is a heartbeat rhythm that varies by more than 25% from the average heartbeat rhythm detected while the unit is measuring the systolic and diastolic blood pressure.

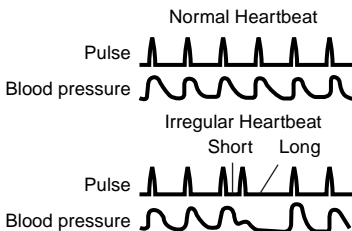


If such an irregular rhythm is detected more than twice during measurement, the irregular heartbeat symbol () appears on the symbol when the measurement results are displayed.


What is Arrhythmia?

A heartbeat is stimulated by electrical signals that cause the heart to contract.

Arrhythmia is a condition where the heartbeat rhythm is abnormal due to flaws in the bio-electrical system that drives the heartbeat. Typical symptoms are skipped heartbeats, premature contraction, an abnormally rapid (tachycardia) or slow (bradycardia) pulse. This can be caused by heart disease, aging, physical predisposition, stress, lack of sleep, fatigue etc. Arrhythmia can only be diagnosed by a doctor through a special examination.

Whether the appearance of the irregular heartbeat symbol () in the results indicates arrhythmia or not can only be determined by an examination and diagnosis by your doctor.

Warning:

If the irregular heartbeat symbol () is shown frequently, please make your doctor aware of it. Conducting self-diagnosis and treatment based on measurement results is dangerous. Be sure to follow the instructions of your doctor.

3.3 Using the Memory Function

The monitor is designed to store the blood pressure and the pulse rate in the memory for two people (user A and user B) every time a measurement is completed.


The monitor automatically stores up to 100 sets of measurement values (blood pressure and pulse rate) for each user (A and B). The monitor also displays an average reading based on the three most recent sets of measurement values taken within 10 minutes of the most recent reading.

Notes:

- To ensure that the measurement results are recorded correctly, make sure that the date and time are set correctly before taking a measurement.
- When 100 sets of readings are stored in memory, the oldest set will be deleted to store a new set.
- The date and time of stored readings will be alternately displayed.


To View the Average Value

Press the MEM button.



To View Previous Readings Stored in Memory

1. Press the MEM button, while the average reading is displayed, to view readings stored in memory from the most recent to the oldest.

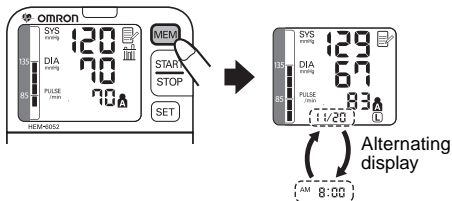


2. Press the MEM button repeatedly to cycle through the readings.

To Delete All Values in Memory









The values stored in the memory are deleted by user ID. You cannot partially delete values stored in the memory. All values for the user you select will be deleted.

When the memory symbol (📄) appears, first press the MEM button, then while holding it down, press the START/STOP button simultaneously for more than 2-3 seconds.

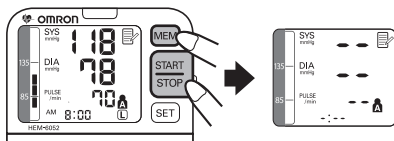

4. Handling Errors and Problems


Symptom	Cause	Correction
No display appears when the START/STOP button is pressed.	Batteries are empty.	Replace with new batteries.
	Batteries were inserted incorrectly.	Insert the batteries with the correct [+] [-] polarity.
Cannot measure or readings are too high.	The wrist cuff is not at heart level.	Measure while in the correct posture. Refer to section 3.2.
	The wrist for measurement is not set appropriately.	Make sure that the setting is set correctly for the wrist being used to take the measurement. Refer to section 3.2.
	The cuff is not wrapped snugly around the wrist.	Wrap the cuff correctly. Refer to section 3.1.
	Your arms and shoulders are tense.	Relax and try taking the measurement again.
	Movement or talking during measurement.	Keep still and do not talk during measurement.
There is no pressure but a reading still appears when the START/STOP button is pressed.	You are in memory mode.	Turn power off once and restart measurement.
The blood pressure is different each time. The reading is extremely low (or high).	Blood pressure readings constantly vary with time of measurement and nervous condition. Take deep breaths to relax before taking a measurement.	

Error Symbol	Cause	Correction
	Cuff is over inflated.	Press the START/STOP button once to turn off the power. Sit still, restart measurement and do not talk during measurement.
	Movement during measurement	Carefully read and repeat the steps in section 3.2. Make sure that the setting is set correctly for the wrist being used to take the measurement.
	The posture has changed during measurement.	
	The wrist cuff is not wrapped securely.	Carefully read and repeat the steps listed under section 3.1.
	The user ID has changed during measurement.	Do not change the user ID during measurement.
	This symbol indicates irregular or weak pulses are detected, but result can be considered reliable.	Remove the monitor. Wait 2-3 minutes and then take another measurement. Repeat the steps in section 3.2. If this error continues to appear, consult your doctor.
	An Er mark is displayed.	Consult your OMRON retail outlet or distributor.
	The battery power is low.	Replace the batteries with two new "AAA" alkaline (LR03) batteries.

5. Storage and Maintenance

To protect your monitor from damage, please avoid the following:


- Subjecting your monitor to extreme temperatures, humidity, or direct sunlight.
- Washing the cuff or exposing the cuff or monitor to water.
- Disassembling the monitor.
- Subjecting the monitor to strong shocks or vibrations. Do not drop the monitor.
- Cleaning the monitor with volatile liquids. The MONITOR SHOULD BE CLEANED WITH A SOFT, DRY CLOTH.

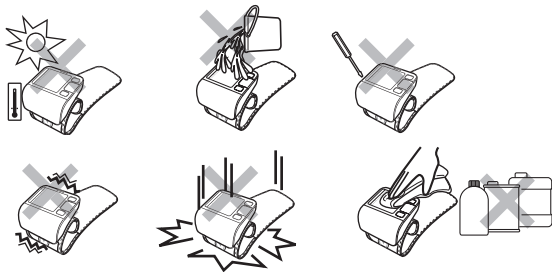

Calibration and Service

- The accuracy of this blood pressure monitor has been carefully tested and is designed for a long service life. It is generally recommended to have the monitor inspected every two years to ensure correct functioning and accuracy. Please consult your authorised OMRON dealer.
- If the wrist cuff needs to be replaced have this done by an authorised expert. Consult your local authorised OMRON distributor or dealer.
- Do not carry out any repairs yourself. If a defect occurs or you have doubts about the correct functioning of the device, consult your local authorised OMRON distributor or dealer.

6. Technical Data

Name	OMRON Wrist Blood Pressure Monitor
Model	HEM-6052
Display	LCD Digital Display
Measurement	Oscillometric method
Measurement Range	Pressure: 0 to 299 mmHg/ Pulse: 40 to 180 beats/min
Memory	100 Measurements with date and time for each user (A and B)
Accuracy	Pressure: Within ± 3 mmHg Pulse rate: Within $\pm 5\%$ of reading
Inflation	Automatic inflation by pump
Deflation	Automatic rapid deflation
Power Source	Two 1.5V "AAA" alkaline (LR03) batteries
Battery Life	Approximately 300 measurements when using alkaline (LR03) batteries at a room temperature of 23°C
Applied Part	 = Type B
Protection Against Electric Shock	Internally powered ME equipment
Operating Temperature/ Humidity	10°C to 40°C, 30 to 85% RH
Storage Temperature/ Humidity/ Air pressure	-20°C to 60°C, 10 to 95% RH, 700-1060 hPa
Weight of Main Unit	Approximately 114 g (not including batteries)
Outer Dimensions	70 mm (w) x 70 mm (h) x 21mm(d) (not including the wrist cuff)
Measurable circumference of wrist	Approximately 13.5 to 21.5 cm
Package Content	Main unit, storage case, two "AAA" alkaline (LR03) batteries, instruction manual, and quick reference guide

Notes:

- Subject to technical modification without prior notice
- Disposal of this product and used batteries should be carried out in accordance with the national regulations for the disposal of electronic products.

CE0197

- This device fulfils the provisions of EC directive 93/42/EEC (Medical Device Directive).
- This blood pressure monitor is designed according to the European Standard EN1060, Noninvasive sphygmomanometers Part 1: General Requirements and Part 3: Supplementary requirements for electromechanical blood pressure measuring systems.

Important information regarding Electro Magnetic Compatibility (EMC)

With the increased number of electronic devices such as PC's and mobile (cellular) telephones, medical devices in use may be susceptible to electromagnetic interference from other devices. Electromagnetic interference may result in incorrect operation of the medical device and create a potentially unsafe situation.

Medical devices should also not interfere with other devices.

In order to regulate the requirements for EMC (Electro Magnetic Compatibility) with the aim to prevent unsafe product situations, the EN60601-1-2:2007 standard has been implemented. This standard defines the levels of immunity to electromagnetic interferences as well as maximum levels of electromagnetic emissions for medical devices.

This medical device manufactured by OMRON HEALTHCARE conforms to this EN60601-1-2:2007 standard for both immunity and emissions.

Nevertheless, special precautions need to be observed:

- Do not use mobile (cellular) telephones and other devices, which generate strong electrical or electromagnetic fields, near the medical device. This may result in incorrect operation of the unit and create a potentially unsafe situation. Recommendation is to keep a minimum distance of 7 m. Verify correct operation of the device in case the distance is shorter.

Further documentation in accordance with EN60601-1-2:2007 is available at OMRON HEALTHCARE EUROPE at the address mentioned in this instruction manual.

Documentation is also available at www.omron-healthcare.com.

Correct Disposal of This Product (Waste Electrical & Electronic Equipment)

This marking shown on the product or its literature, indicates that it should not be disposed of, with other household wastes at the end of its working life. To prevent possible harm to the environment or human health from uncontrolled waste disposal, please separate this from other types of wastes and recycle it responsibly to promote the sustainable reuse of material resources.

Household users should contact either the retailer where they purchased this product, or their local government office, for details of where and how they can take this item for environmentally safe recycling.

Business users should contact their supplier and check the terms and conditions of the purchase contract. This product should not be mixed with other commercial wastes for disposal.

This product does not contain any hazardous substances.



7. Some Useful Information about Blood Pressure

What is Blood Pressure?


Blood pressure is a measure of the force of blood flowing against the walls of the arteries. Arterial blood pressure is constantly changing during the course of the heart's cycle. The highest pressure in the cycle is called the *Systolic Blood Pressure*; the lowest is the *Diastolic Blood Pressure*. Both pressure readings, the *Systolic* and *Diastolic*, are necessary to enable a doctor to evaluate the status of a patient's blood pressure.

Why is it a Good Thing to measure Blood Pressure at Home?

Having your blood pressure measured by a doctor can cause anxiety which is itself a cause of high blood pressure. As a variety of conditions affect blood pressure, a single measurement may not be sufficient for an accurate diagnosis. Many factors such as physical activity, anxiety, or the time of day, can influence your blood pressure. Thus it is best to try and measure your blood pressure at the same time each day, to get an accurate indication of any changes in blood pressure. Blood pressure is typically low in the morning and increases from afternoon to evening. It is lower in the summer and higher in the winter.

Blood pressure is measured in millimetres of mercury (mmHg) and measurements are written with the systolic pressure before the diastolic e.g. A blood pressure written as 140/90, is referred to as 140 over 90 mmHg.


7. Some Useful Information about Blood Pressure

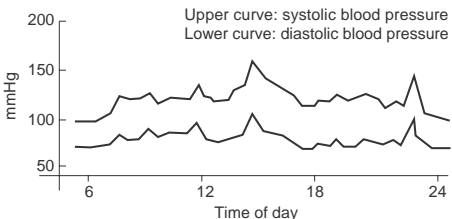

Example: fluctuation within a day (male, 35 years old)



Classification of Blood Pressure by the World Health Organization

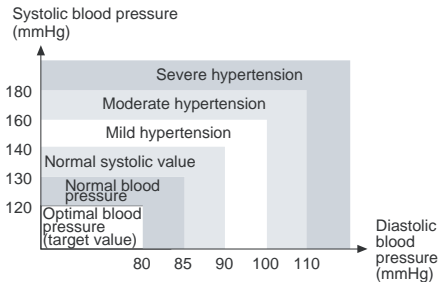The World Health Organization (WHO) and the International Society of Hypertension (ISH) developed the Blood Pressure Classification shown in this figure.



This classification is based on the blood pressure values measured on people in a sitting position in outpatient departments of hospitals.

*There is no universally accepted definition of hypotension. However, those having the systolic pressure below 100 mmHg are assumed as hypotensive.

	<p>OMRON HEALTHCARE Co., Ltd. 24, Yamanouchi Yamanoshita-cho Ukyo-ku, Kyoto, 615-0084 JAPAN</p>
	<p>OMRON HEALTHCARE EUROPE B.V. Kruisweg 577, 2132 NA Hoofddorp THE NETHERLANDS</p>
<p>Asia Pacific HQ</p>	<p>OMRON HEALTHCARE SINGAPORE PTE LTD. 438A Alexandra Road, #05-05/08, Alexandra Technopark, Singapore 119967</p>